“Impala (Economic)”
Item nr. 312060 and 312061

User's manual

CE

MOBILEX A/S
Grønlandsvej 5
DK-8660 Skanderborg
Denmark
www.mobilex.dk

1. General information

Dear customer,

This user manual contains a description of the medical device and important guidances to ensure a correct and safe usage of the product. It is important prior to use to read this manual carefully. It is especially important to read the safety requirements and follow these.
We continuously develop our products and we reserve the right without further notice to change the specifications and functions of products.

Intended use of the device
The Mobilex Product is medical device which is intended to be used only as a walking assistant by patients that because of invalidity are unable to stand, walk or sit independently and who require additional stable support during walking. It gives for such persons possibility to fulfil most of their regular, daily activities without the assistance of a helper.

Any other use is prohibited

Indications: the device is indicated for use as walking, standing and seating support by persons who suffer different diseases of human motion system. The variety of such diseases is very wide but the symptoms are similar: people who because of their health status are unable to walk, stand or sit independently are indicated to use rollators. The final decision to choose the correct type of device depends on condition of individual patient and should always be taken by professional physician or physical therapist

With questions please take contact to your dealer or directly to Mobilex A/S.

Mobilex A/S
Grønlandsvej 5
DK-8660 Skanderborg
Denmark

Phone: +45 87 93 22 20
Telefax: +45 87 93 17 77
E-Mail: info@mobilex.dk

2. Safety requirements

- Only use the product in flawless condition.
- If defects or errors are detected you must immediately contact the dealer.
- Follow the information on the product label.
- Only use the product for the described purpose.
- Avoid making constructive changes on the device, unless you have the manufacturer’s written acceptance for such modifications.
- During different adjustments which are possible on the device the user must take care not to squeeze the fingers or other body parts between two moving elements of the device
- The device must only be used on a stable surface.
- All wheels MUST be in contact with the floor at ALL TIMES during use. This will ensure the rollator is properly balanced and should avoid accidents.
- When using the rollator in a stationary position, the hand brakes MUST be locked.
- The device must not be loaded with more than max load value described in Technical Data and on product's label.
- The device’s basket has load limitation of 5 kg.
- The device is dedicated to be used indoor or outdoor on flat surfaces.
- The device is not intended to be self-propelled while seated
- The brakes MUST be in the locked position BEFORE using the seat.

3. Description

Product description
The rollator is made o powder coated steel frame with plastic seat and push handles. It offers great manoeuvrability, stability and it has height adjustable push handles for a user fit. It is equipped with comfortable seat and back support, so the device allows the user to rest. The basket eliminate the need to hand carry items.

Mobilex A/S
Grønlandsvej 5
DK-8660 Skanderborg
www.mobilex.dk

Rollators are supplied in cartons, detached in to few elements for easier transportation:
The contents are:

- 1 Main Frame with wheels, shopping basket and seat
- 2 Detachable Push Handles with Brake Handles attached
- 1 Detachable backrest bar
- 1 User's manual

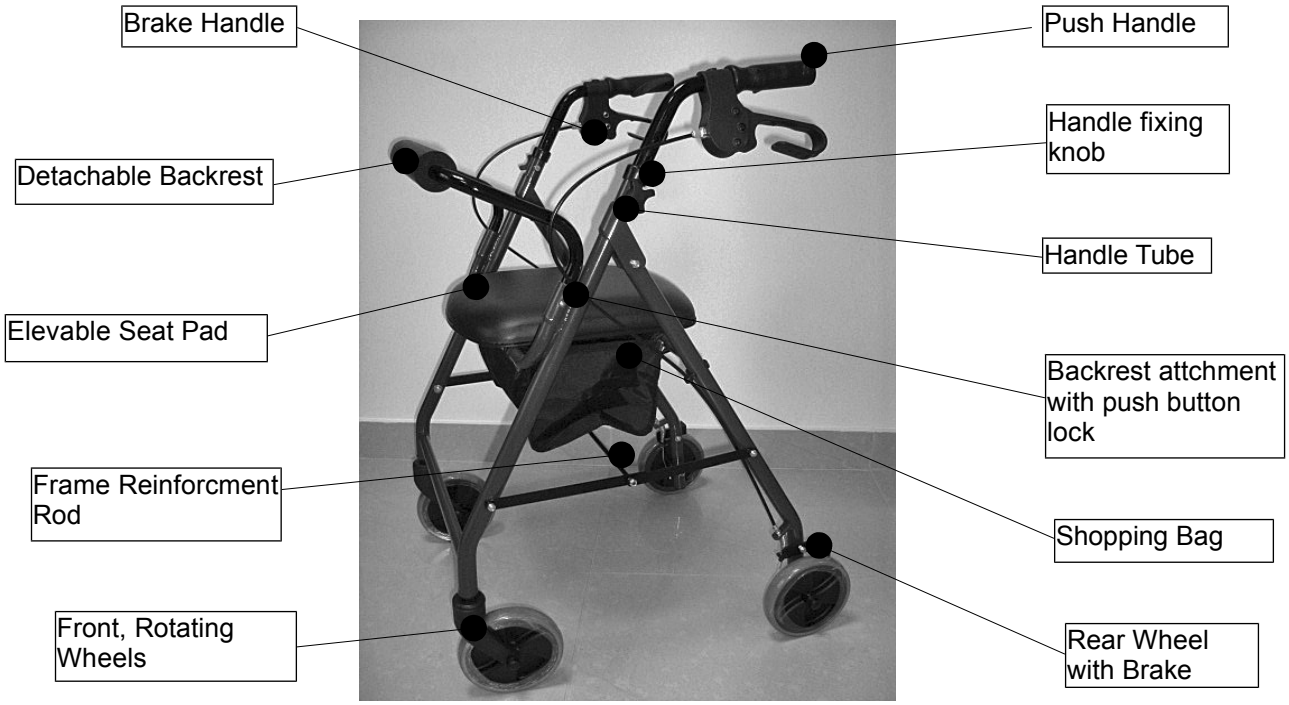

Assembly description

- Check with the list from above if nothing is missing. If you'd discover at that stage that some part is missing or damaged, do not continue assembly process. Contact your supplier of the product right away.
- Put the main frame with wheels on the flat surface. All wheels should touch the floor.
- Press the frame reinforcement rod downwards until the frame is fully opened. Push the seat pad down, so it is in horizontal position
- Always ensure the frame is stable and fixed when the rollator is opened.
- Insert the lower ends of push handles in to holes at the top of handle tubes as it is shown on picture above.
- Adjust both push handles to the same height. Ensure that the fixing holes in the push handle and in the handle tube are parallel.
- Put the bolt the fixing bolt through the parallel holes. Do it from the inside of the frame so the fixing knob should be located on the outside. Tie the fixing knobs on the handle tubes as shown on the picture above.
- Make sure that the fixing knobs (2 pieces) are securely locked so that the rollator is stable and parts can not move when forced.
- Attach the backrest. Insert the backrest tube ends in to backrest attachements located on main frame as shown on the picture. You should hear the ”click”sound to ensure that the back is safely locked.
- Always test to see that the rollator and attachments are properly and safely locked in place BEFORE using.
- Failure to follow these warnings can result in personal injury.
- To fold the rollator lift the seat pad first. Then pull the frame reinforcement rod upwards. The frame should fold.

Function description

- Adjust the height of the push handles so that when the user's arm is down along the body, the handles are at wrist height. Adjust the height by releasing the fixing knob located on handle tube and pulling the bolt out of it's place. Then adjust supports to your desired

height, then have the bolt go through the holes and tie thr knob securely. Repeat the steps for the other handle, so both are at the same height.

- Care should be taken to ensure that ALL adjustments are secured and that castors and moving parts are in good working order before using.
- To stop the rollator simply pull the brake handles up towards hand grips and hold brake handles in the ”UP” position to remain stationary. TO MOVE simply release the brake handles.
- To lock the brakes in ”engaged” position for longer period of ”parking”push the brake handles down until you can hear the ”click” sound. To unlock the brakes pull the brake handles UP again until you can feel them loose.
- While using the rollator in a stationary position, the hand brakes MUST always be locked. You should always engage the breaks when you don’t plan to move the device. Never leave device without breaks engaged when there is someone sitting in it! Never leave device on slopes without breaks engaged!

Transport recommendations
The rollator is an easily foldable product convenient for transportation. If it is necessary to transport it, we recommend to fold it as it is written in description above. Rollator should be transported in the way that it is stable and there is no risk of sudden and dangerous movements of the transported device.

Accessories
There are no accessories provided for this device

4. Technical data

Technical data	Item nr. 312060 Standard	Item nr. 312061 Large
Height over all / height of the push handles (adjustable)	78 - 93 cm	90 - 104,5 cm
Total width	61 cm	63,5 cm
Total length (opened)	70 cm	74,5 cm
Total length (folded)	33 cm	33 cm
Seat height	53 cm	63 cm
Seat width (internal width)	44 cm	46 cm
Width of the padded seat	35,5 cm	35,5 cm
Depth of the padded seat	32,5 cm	32,5 cm
Max. Load	120 kg	150 kg
Max. Load of the bag	5 kg	5 kg
Weight	7,5 kg	8,2 kg
Brakes	2 lockable	2 lockable

Product label
The product label is located on the frame tube.

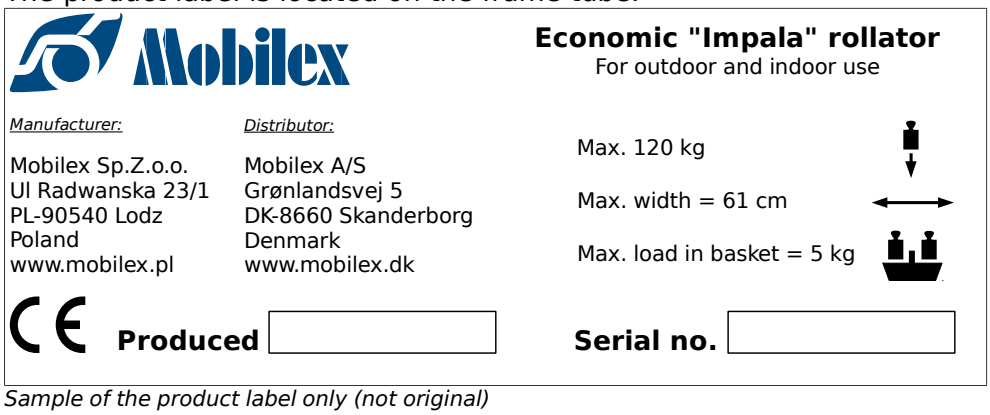

Sample of the product label only (not original)

Mobilex A/S
Grønlandsvej 5
DK-8660 Skanderborg
www.mobilex.dk

5. Maintenance & Cleaning

Regularly clean the device and keep it clean. Normal dirt on metal and plastic parts can be removed with wet cloth and standard, non-corroding, mild washing cleaning agents. Check the specific product information and use only commercial cleaning products which are suitable for cleaning and disinfection (Do not use solvents, harsh abrasives or bleach based cleaners). Dry parts with soft cloth.

Lubricate wheels' axles with 3-in-1 oil periodically or if wheels begin to squeak. Ensure that every part of the rollator is secure at ALL times. Check all screws for tightness. If not. Tighten if necessary. Replace any broken, damaged or worn items immediately.

Despite the solid construction and the use of resistant materials the product is subject to wear. It is therefore recommended to let check the product at regular intervals by a professional

6. Most common problems and solutions

Symptoms	*possible cause*	*what to do?*
The wheels don't turn smooth and easily	There is a dirt between wheels and forks	Clean the space between wheels and forks. Lubricate the axles of the wheels
Brakes aren't working correctly or one brake works stronger than the other.	The brake foot is torn or brake cable isn't adjusted correctly	Replacement of brake foot or cable adjustment required. Contact the service centre.

7. Disposal of the product

The product can not be disposed of with household waste but must be brought to the local recycling centre.

8. Guarantee terms

Mobilex A/S offers 2 years of guarantee for damages caused by errors in production. The guarantee is not valid by not-intended use of the product. Parts subject to normal wear are not covered by the guarantee, unless wear is caused by a manufacturing fault. In the event of damage, please notify your dealer. The guarantee does not cover transport cost. The guarantee does not cover injury or other damages eventually related to a malfunction of this product.

9. Declaration of Conformity (CE)

The company Mobilex A/S, Grønlandsvej 5, 8660 Skanderborg, Denmark declares that the product

”Impala (Economic)” Rollator 312060 and 312061

is designed in accordance with the technical documentation and made of which conforms to the following basic requirements:

- **EU Council Directive 93/42/EEC for medical equipment Annex I of the June 14, 1993**

Lars Nygaard
Managing Director
Mobilex A/S

Skanderborg, the 2011.12.10

.....
signature